

---

## Urgent Field Safety Notice

**Subject:** Liko® Overhead and Mobile Lifts—Standard SlingBar™ 450

**FSCA-identifier:** Mod 486

**Type of action:** Device Modification

---

**Date:**

**To:** Chief Executive, Facility Administrator, Facility Engineer, Vigilance Manager  
Biomedical Engineering, Medical Device Liaison Officer

**Affected Devices:** Standard SlingBar™ 450, product numbers: 20090029, 20190024, 20190041, 31190015, 31290017, 31290043, 3156001, 3156003, 3156007, 3156014, 3156016, 31590043 or 5019013  
**distributed between January 1980 and November 2012**


These product numbers may be bundled with the Golvo 1000, 3000, and 7000 series lifts, Viking M, Viking L, LikoLight 100 & 125, Caroli 101, and Uno 100, 101 & 102.

**Background:**


Hill-Rom has become aware of a safety issue related to the Standard SlingBar™ 450, which could be attached to various Liko overhead and mobile lifts. A serious injury to a patient, caregiver, or bystander could result from tripping or otherwise falling in to the slingbar, typically while the lift is parked or stored when not in use. The sling hook on the end of the slingbar could pierce a body structure such as the head, shoulder, or groin.

There have been five serious injuries resulting from persons tripping or falling into the slingbar. There has been one serious injury from a person climbing on/playing with the lift. There are no malfunctions with the device associated with these incidents.

Hill-Rom has developed a slingbar safety cover to mitigate these risks (see illustration on next page).

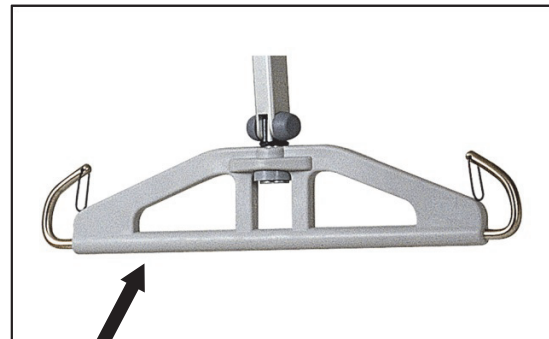

**This style slingbar ONLY is affected.**

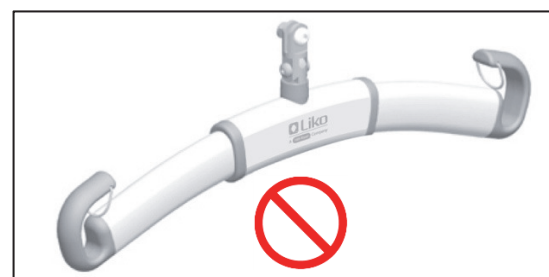


**Universal Slingbar is NOT affected.**

**Action to be taken by user:**

Included with this notification is a **Response Form**. Please determine the number of slingbar safety covers that you need, **complete and return the form to Hill-Rom as soon as possible**, and we will send you the applicable number of kits to you at no cost.

Continue to follow safe lifting practices, and do not allow unauthorized persons, especially children, to play around or operate the lift.

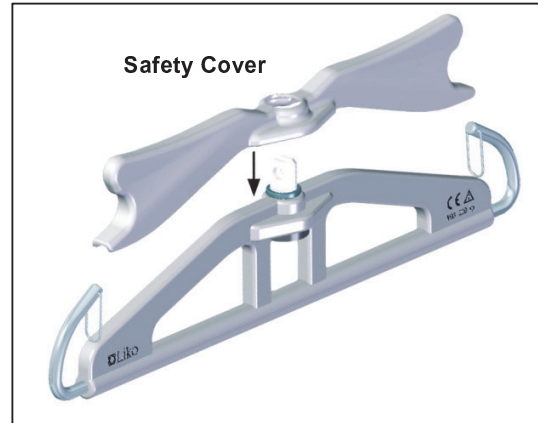

**Safety Cover Illustration**

**Transmission of this Field Safety Notice:**

Please forward a copy of this letter to any other facility personnel you deem appropriate.

Please maintain awareness of this notice and resulting action for an appropriate period to ensure effectiveness of the corrective action.

Hill-Rom confirms that the relevant Competent Authorities have been informed of this Field Safety Corrective Action.

**Contact reference person:**

If you have any questions concerning this Safety Notice, please contact Hill-Rom Technical Support, your Distributor, or your Hill-Rom representative.

Regards,

Hill-Rom Technical Support

Attachment: Response Form



## Response Form

**Subject: Liko® Overhead and Mobile Lifts—Standard SlingBar™ 450  
(Mod 486)**

Please complete the following with the correct information, and **return this Response Form** without delay to Hill-Rom Technical Support. See specific instructions at bottom of page. Thank you.

---

Liko account number: \_\_\_\_\_

Name of the facility: \_\_\_\_\_

Address of the facility: \_\_\_\_\_

City: \_\_\_\_\_ State: \_\_\_\_\_ Zip: \_\_\_\_\_

Facility Authorized Name: \_\_\_\_\_

*Please print legibly*

Signature: \_\_\_\_\_

Title: \_\_\_\_\_ Date: \_\_\_\_/\_\_\_\_/\_\_\_\_ Phone: \_\_\_\_\_

Fax: \_\_\_\_\_

Check action taken:

- We do not have any affected products.
- We need \_\_\_\_\_ safety covers to retrofit all affected slingbars in our facility.

**As soon as possible,  
please FAX or email this form to:**