



M.A. ARAIN & BROTHERS (PVT.) LTD.

Manufacturers & Exporters of fine quality Surgical, Electrosurgical & Diagnostic Instruments

Urgent Field Safety Notice

Catalogue Numbers of Teleflex

Date:15.03.2013

670160-0000** (Laryngoscope disposable metallic kit)

670190-0000** (Laryngoscope disposable metallic kit)

670195-0000** (Disposable Laryngoscope battery handles)



ISO 9001:2008



ISO 13485:2003



ISO 14001:2004



CE

CERTIFIED

Extension of Recall M. A. Arain & Brothers (Pvt) Ltd Reference Number: MB/509/13/04

LOT-Number of affected Products:

- 031511
- 040811 - This Field Safety Corrective Action affects this LOT-Number which is not indicated on the label of the products. Therefore, if no LOT number is identified the products are affected.
- 041511
- 011012
- 020712
- 021512
- 030812
- 032112
- 040412
- 040912
- 042712
- 052912

Description of the problem:

During examination of a complaint it was discovered that some coil springs in the battery compartment were improperly engaged during manufacturing. It most likely will be discovered before the application but it may happen during intubation.

MEMBERS



MAILING ADDRESS: P.O. BOX 432, SIALKOT-PAKISTAN
FACTORY: WAZIRABAD ROAD, SIALKOT.
TEL: +92-52-4264926, 4264571 FAX: +92-52-4264759, 4264026
E-mail: info@maarain.com URL: <http://www.maarain.com>



M.A. ARAIN & BROTHERS (PVT.) LTD.

Manufacturers & Exporters of fine quality Surgical, Electrosurgical & Diagnostic Instruments




Advise on action to be taken by the user:

Stop using the above indicated products immediately. Please send back affected products for replacement and check similar other products intend to the same issue before use.

Transmission of this Field Safety Notice:

This needs to be passed on all those who need to be aware within your organization or to any organization where the potentially affected devices have been transferred. (If appropriate)

The undersigned confirms that the appropriate competent authorities have been advised of the FSCA.

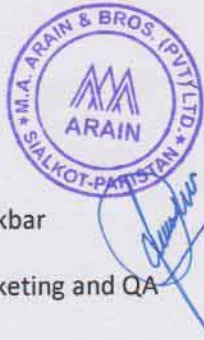

Mr. Waqas Akbar

Director Marketing and QA

MEMBERS



MAILING ADDRESS: P.O. BOX 432, SIALKOT-PAKISTAN
FACTORY: WAZIRABAD ROAD, SIALKOT.
TEL: +92-52-4264926, 4264571 FAX: +92-52-4264759, 4264026
E-mail: info@maarain.com URL: http://www.maarain.com