



Public Health
England

Results of the 2013 PHE Intercomparison of Passive Radon Detectors

About Public Health England

Public Health England exists to protect and improve the nation's health and wellbeing, and reduce health inequalities. It does this through advocacy, partnerships, world-class science, knowledge and intelligence, and the delivery of specialist public health services. PHE is an operationally autonomous executive agency of the Department of Health.

Public Health England
133–155 Waterloo Road
Wellington House
London SE1 8UG
T: 020 7654 8000

www.gov.uk/phe

Twitter: [@PHE_uk](https://twitter.com/PHE_uk)

Facebook: www.facebook.com/PublicHealthEngland

© Crown copyright 2014

You may re-use this information (excluding logos) free of charge in any format or medium, under the terms of the Open Government Licence v2.0. To view this licence, visit OGL or email psi@nationalarchives.gsi.gov.uk. Where we have identified any third party copyright information you will need to obtain permission from the copyright holders concerned.

Any enquiries regarding this publication should be sent to

Press and Information
Centre for Radiation, Chemical and Environmental Hazards
Public Health England
Chilton, Didcot, Oxfordshire OX11 0RQ
E: ChiltonInformationOffice@phe.gov.uk

Published August 2014

PHE publications gateway number: 2014175

Results of the 2013 PHE Intercomparison of Passive Radon Detectors

Z Daraktchieva, C B Howarth and R Algar

ABSTRACT

Intercomparison exercises for passive radon detectors have been held regularly by PHE and its predecessor organisations over many years. In 2013, 25 laboratories from 12 countries, took part in the exercise. Some laboratories submitted more than one set of detectors. A total of 31 sets of detectors were exposed in the PHE radon chamber.

The detectors were exposed to five different radon concentrations ranging from 50 to 3000 kBq m⁻³ h. After exposure, the detectors were returned to the originating laboratories for processing. Each participant was asked to return results for each detector in terms of exposure to radon. A parameter referred to as measurement error, was used to evaluate the performance for each exposure separately and to classify results. Results have been reported to individual participants and are presented here.

EXECUTIVE SUMMARY

Radon is the largest and most variable contributor of radiation dose to the general population. For more than 20 years, countries in Europe and elsewhere have carried out surveys in order to determine both individual and average exposures and identify where excessive exposures might occur. Most of these measurements have been carried out using passive etched track radon detectors exposed for periods of months. Activated charcoal and electret radon detectors have also been used, mainly for shorter term measurements. In addition, all three types of detector are used for experimental and research work.

Intercomparisons provide information about the accuracy of measurements. By allowing different detectors to be compared side by side, an objective assessment of the accuracy of measurements can be made. The results of intercomparisons have been used by individual laboratories to identify and rectify problems, as well as providing calibrations for their detectors traceable to international standards.

The Centre for Radiation, Chemical and Environmental Hazards of Public Health England (CRCE) carries out international laboratory intercomparisons of passive radon detectors each year. For this intercomparison laboratories were invited to submit sets of detectors that were randomised into six groups at CRCE. Five of these groups were exposed in the CRCE radon chamber to five different radon concentrations ranging from 50 to 3000 kBq m⁻³ h and the sixth group was used to determine transit exposures. The detectors were then returned to the laboratories who were asked to report the integrated exposure result for each detector. The laboratories were not informed of the details of the exposures or which detectors were in which group until all the results had been submitted.

This report considers the results for the intercomparison carried out in 2013, for which a total of 25 laboratories from 12 countries submitted 31 sets of detectors. Analysis of the results allows each exposure group in each set to be classified from A (best) to F (worst). All types of detector, whether etched track or electret, can be found in each class, demonstrating the point that, in measuring radon, stringent quality assurance is vital irrespective of the measured technique.

CONTENTS

Abstract	i
Executive Summary	iii
1 Introduction	1
2 Laboratory Exposure and Measurement Facilities	2
3 Logistical Arrangements	2
4 Radon Exposures	2
5 Performance classification Scheme	3
6 Results and Discussion	4
7 Conclusion	5
8 Acknowledgements	5
9 References	5
10 List of Participants	6
11 Tables and Figures	7

1 INTRODUCTION

Passive detectors, of varying designs have been used for many years to make measurements of integrated radon exposures. The three most common methods are outlined below.

- a** Etched track detectors are referred to as such because alpha particles from the decay products of radon damage the surface of the plastic detection medium producing microscopic tracks. These tracks are subsequently made visible by chemical or electrochemical etching. The most popular etched track materials are cellulose nitrate (LR-115), polycarbonate (Makrofol) and polyallyl diglycol carbonate (CR-39). In the open type of etched track detector the plastic material is exposed to the ambient atmosphere. Open etched track detectors record alpha particles originating from radon decay products and from radon isotopes. For these detectors, the radioactive decay equilibrium factor, F , for radon-222 has to be taken into account to estimate the proportion of alpha particles that arise from radon-222 decay. In the closed type, the detection material is enclosed in a chamber that excludes entry of ambient radon decay products and only allows entry of radon gas by diffusion
- b** Activated charcoal detectors work by retaining adsorbed radon in a charcoal volume. The radon is subsequently measured in the originating laboratory
- c** Electret detectors consist of an air chamber above an electret. Ionisation of air in the chamber by radon gradually discharges the electret. Measurement of the charge on the electret by the laboratory before and after radon exposure allows the average radon concentration during exposure to be calculated

Passive radon detectors are quite simple to produce and process but each is subject to sources of error. It is therefore appropriate for laboratories that use these detectors to undertake regular checks against reference exposures carried out in relevant radon exposure facilities. The present laboratory intercomparison programme, which was developed with broad international participation, following standard and agreed test and interpretation protocols, has been designed to provide participants with a routine benchmark performance standard. The intercomparison programme was established by the National Radiological Protection Board (NRPB)* and has operated regularly since 1982. It is now run by the PHE Centre for Radiation, Chemical and Environmental Hazards (CRCE).

Operational procedures and equipment have been described previously (Howarth, 2009; Daraktchieva et al, 2012).

* The NRPB was subsequently incorporated into the Health Protection Agency (HPA). On 1 April 2013 the HPA was abolished and its functions transferred to Public Health England.

2 LABORATORY EXPOSURE AND MEASUREMENT FACILITIES

The exposures in this intercomparison were carried out in the CRCE radon chamber. This 43 m³ walk-in chamber is of the static type, in which radon is continuously released from dry radium-226 radon sources. There is no air flow through the chamber during operation.

The radon atmosphere in the chamber can be varied from around 200 to 8000 Bq m⁻³. Table 1 shows the parameters measured and controlled in the chamber

The radon concentration in the chamber was continuously monitored using an ATMOS 12 DPX ionisation chamber and with an Alphaguard ionisation chamber as a second primary transfer standard. A daily cross-calibration between the Atmos12 DPX and Alphaguard was carried out throughout the intercomparison exercise. Both instruments are calibrated regularly using a radon gas source supplied by Physikalisch Technische Bundesanstalt (PTB), Germany.

During exposures, radon decay products were sampled approximately five times per day on to a Millipore AA filter and their concentrations determined using an alpha spectrometry system. All chamber-monitored data was automatically transferred to a database. Radon and radon decay product exposures were calculated subsequently.

3 LOGISTICAL ARRANGEMENTS

In total, 25 laboratories from 12 countries, took part in the 2013 PHE intercomparison. Some laboratories submitted more than one set of detectors, so 31 sets of detectors were exposed in the radon chamber. Following exposure, the detectors were returned to the originating laboratories for processing. Each participant was asked to return results for each detector in terms of exposure to radon. Participants were not told any details of the exposures delivered in the exercise.

4 RADON EXPOSURES

Appropriate conditions were established in the chamber before introducing the detectors. An equilibrium factor, *F*, of about 0.46 between radon and its decay products was maintained in the chamber for the five intercomparison exposures. The chamber exposures were calculated after the deadline for return of results by participants and are shown with exposure durations in Table 1. Radon and EER (equilibrium equivalent of radon) concentrations during the exposures are shown in Figures 1–5.

The radon concentration in the laboratory outside the exposure chamber was monitored during the exposures using an Alphaguard ionisation chamber. The daily average concentrations ranged from 23 to 48 Bq m⁻³, with an overall average of 33 Bq m⁻³. The estimated additional exposure of the detectors caused by leaving them exposed in the laboratory for three days to allow radon to diffuse out of them was less than 1% of the exposure in the chamber in all cases and the values were neglected for the purpose of calculating the reference exposures. Transit detectors were used to monitor radon exposure received in transit.

5 PERFORMANCE CLASSIFICATION SCHEME

A performance classification scheme was introduced in 2011 based on the following parameters:

- a** Percentage biased error, which measures the bias of the measurement
- b** Percentage precision error, which measures the precision of the measurement
- c** Percentage measurement error, which takes into account their combined effect

The measured mean is obtained by subtracting the mean transit exposure from the mean reported exposure.

The parameters are given below:

$$\% \text{ biased error} = \frac{\text{Measured mean} - \text{Reference value}}{\text{Reference value}} \times 100$$

where the reference value is the reference radon exposure,

$$\% \text{ precision error} = \frac{\text{Standard deviation}}{\text{Measured mean}} \times 100$$

$$\% \text{ measurement error} = \sqrt{\% \text{ biased error}^2 + \% \text{ precision error}^2}$$

Since the percentage measurement error combines the biased error and precision error, a result can have low measurement error only if both bias and precision errors are low. Measurement errors are reflected as a performance classification from A (best) to F (worst) for each exposure separately. Each participating laboratory is assigned a classification, between A and F, for each exposure. The criterion for each of the classification groups is given below.

Range of measurement error (%)	Performance classification
< 10%	A
≥ 10% and < 20%	B
≥ 20% and < 30%	C
≥ 30% and < 40%	D
≥ 40% and < 50%	E
≥ 50%	F

6 RESULTS AND DISCUSSION

The results reported by the laboratories are given in Table 2. In these tables, the ‘mean’ is the mean result of ten exposed detectors (five for electrets) after subtracting the mean transit exposure. The standard deviation, ‘1 SD’, is for ten reported results (five for electrets). Results for % biased error, % precision error and % measurement error are provided as well.

The mean results and their standard deviations, as reported by participants, are depicted in Figures 6–10. The mean of all transit exposures is shown in Figure 11. Analysis showed that the reported results were nearly normally distributed for all five exposures. The mean, μ , and standard deviation, σ , of all reported results, calculated for each exposure, are given in Table 3. The distributions of the mean exposure results given in Table 3 are depicted in Figure 12.

The characteristics of the detectors such as material, detector holder design, detector type and material supplier are provided in Table 4.

The mean of all transit exposures is $34 \text{ kBq m}^{-3} \text{ h}$ (Figure 11). Most of the reported transit exposures were below $50 \text{ kBq m}^{-3} \text{ h}$, three laboratories reported values between 50 and $100 \text{ kBq m}^{-3} \text{ h}$, while two laboratories reported values above $100 \text{ kBq m}^{-3} \text{ h}$.

Results, using the performance classification scheme, are given in Table 4. This table is sorted according to performance classification with the first order of sort being the lowest exposure. The position of a laboratory in the table reflects the performance classification of the different exposures and should not be interpreted as a criterion of their total performance. The results in the table are informative and can be used by laboratories to review their procedures and to identify problems at different exposure levels.

Six laboratories participating with eight sets of detectors achieved five class A results, meaning that they have a measurement error of under 10% for all five exposures. Moreover, 58% of all sets of detectors achieved class A for exposures 1, 3 and 5 – an improvement over the results achieved in 2011 and 2012. There was also general improvement in performance at measuring the lowest exposure ($144 \text{ kBq m}^{-3} \text{ h}$): 24% of laboratories achieved class A compared with 14% in 2012.

It should be noted that the laboratories participating with the same type of detectors and detector material can achieve quite different performance classifications, possibly reflecting each laboratory’s own quality assurance (QA) protocols.

In order to identify sources of errors, the laboratories should take into account changes in various parameters such as calibration factor, sensitivity and background. Reviews of sources of errors for etched track detectors are given in Ibrahim et al (2009), Hanley et al (2008) and Hardcastle and Miles (1996). Constant monitoring of detector performance and strict QA protocols should be established and maintained to identify and manage the above sources of errors.

The proportion of sets achieving each performance classification (A–F) is given in Figure 13.

7 CONCLUSION

In total, 25 laboratories from 12 countries participated in the 2013 PHE intercomparison of passive radon detectors. A six-band (A–F) classification scheme was used to evaluate the performance of the detectors across a range of exposures.

8 ACKNOWLEDGEMENTS

The authors would like to thank Stefania Harford and Dr Jaroslaw Wasikiewicz who provided valuable assistance in the radon exposure of the detectors.

9 REFERENCES

- Daraktchieva Z, Howarth CB and Algar R (2012). Results of the 2011 HPA Intercomparison of Passive Radon Detectors. Chilton, HPA-CRCE-033.
- Hanley O, Gutierrez-Villanueva JL, Currivan L and Pollard D (2008). Assessment of the uncertainties in the Radiological Protection Institute of Ireland (RPII) radon measurements service. *Journal of Environmental Radioactivity*, **99**, 1578–82.
- Hardcastle GD and Miles JCH (1996). Ageing and fading of alpha particle tracks in CR-39 exposed to air. *Radiation Protection Dosimetry*, **67**(4), 295–8.
- Howarth CB (2009). Results of the 2007 HPA Intercomparison of Passive Radon Detectors. Chilton, HPA-RPD-060.
- Ibrahimi Z-F, Howarth CB, Miles JCH (2009). Sources of error in etched-track radon measurements and a review of passive detectors using results from a series of radon intercomparisons. *Radiation Measurements*, **44**, 750–54.

10 LIST OF PARTICIPANTS

Contact person	Organisation	Country
Dr Nivaldo Carlos da Silva	Brazilian Commission for Nuclear Energy – CNEN Laboratory of Poços de Caldas – LAPOC	Brazil
Renato Falcomer	Health Canada National Radon Laboratory	Canada
Fred Sarradin	Dosirad	France
Pierre Filleul	LED-ALGADE	France
Vincent Delpech	Pearl-SAS (Pôle d'Expertise et d'Analyse Radioactivité Limousin)	France
Maria Kolovou	Department of Environmental Radioactivity - GEAEK	Greece
Eric Hülber	Radosys Ltd	Hungary
Michael Murray	RPII	Ireland
Dr Luca Verdi	Agenzia Provinciale per l'Ambiente	Italy
Chiaberto Enrico	ARPA Piemonte	Italy
Massimo Calamosca	ENEA – IRP-DOS	Italy
Dr G Torri	ISPRA – Servizio Misure Radiometriche	Italy
Dr L Baldassarre	LB Servizi per le Aziende srl	Italy
Dr Marta Rossetti	U-Series Srl	Italy
Daniele Bonamini	Tecnorad s u r l	Italy
Marielle Lecompte	Service d'Analyses Radiologiques – LNS, Ministère de la Santé – Direction de la Santé	Luxembourg
Aleksandar Birovljev	Radonlab Ltd	Norway
Trine Kolstad	NRPA	Norway
Dr Tryggve Rönnqvist	Landauer Nordic AB	Sweden
Professor Gilbert Jönsson	RADONANALYS GJAB	Sweden
Sefa Kemal Uzun	SANAEM	Turkey
Darren Langridge	Dstl Radiological Protection Services	UK
Dr Phil Gilvin	PHE Personal Monitoring Services	UK
Simon Crust	Kingston University, School of Geography, Geology and Environment	UK
Maria Hansen	Track Analysis Systems Ltd	UK

11 TABLES AND FIGURES

TABLE 1 Exposure parameters

Exposure	1	2	3	4	5
Duration (h)	431.4	20.25	192.6	52.63	98.93
Radon exposure (kBq m ⁻³ h)	2990	144	1326	347	657
Uncertainty (%) at 68% CL	3.0	3.0	3.0	3.0	3.0
EER exposure (kBq m ⁻³ h)	1375	60	597	156	335
Uncertainty (%) at 68% CL	7.0	7.0	7.0	7.0	7.0
<i>F</i> _e equilibrium factor	0.46	0.42	0.45	0.45	0.51

Notes

EER is equilibrium equivalent of radon.

CL is the confidence level.

Notes to Table 2 and 4

The results for two detectors in set 16-1 were incorrectly assigned by either PHE or the reporting laboratory. When the corrected results were supplied the results for the mean of exposure 1 and 4 were 2652.2 and 371.0 kBq m⁻³ h, respectively. The measurement errors for exposure 1 and 4 when corrected were 11.4% and 9.1%, respectively. The ranks for exposures 1 and 4 when corrected were B and A, respectively.

All results in set 172-1 were reported with the transit value already subtracted by the reporting laboratory.

The results for two detectors in set 28-1 were incorrectly assigned by the reporting laboratory. When the corrected results were supplied the results for the mean of exposure 1 and 5 were 3167.5 and 654.7 kBq m⁻³ h, respectively. The measurement errors for exposure 1 and 5 when corrected were 7.3% and 4.6%, respectively. The performance classifications for exposures 1 and 5 when corrected were A and A, respectively.

TABLE 2 Analysis of all reported results
Exposure 1 2990 kBq m⁻³ h

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	% biased error	% precision error	% measurement error
7-1	2651.3	80.2	-11.3	3.0	11.7
13-1	2888.2	88.8	-3.4	3.1	4.6
14-1	2806.1	76.4	-6.2	2.7	6.7
16-1	2427.5	727.2	-18.8	30.0	35.4
16-2	2733.3	75.7	-8.6	2.8	9.0
16-3	2763.2	32.9	-7.6	1.2	7.7
19-1	2688	33.6	-10.1	1.3	10.2
20-1	2618	82.6	-12.4	3.2	12.8
23-1	2990.3	127.2	0.0	4.3	4.3
25-1	3560.1	167.1	19.1	4.7	19.6
25-2	3471	346.4	16.1	10.0	18.9
28-1	2921.2	815.0	-2.3	27.9	28.0
32-1	2882	44.4	-3.6	1.5	3.9
40-1	3940.9	358.0	31.8	9.1	33.1
45-1	3016.2	271.3	0.9	9.0	9.0
122-1	3146.3	45.4	5.2	1.4	5.4
122-2	2979	98.5	-0.4	3.3	3.3
129-1	2838.3	72.3	-5.1	2.5	5.7
141-1	3334.6	131.4	11.5	3.9	12.2
144-1	3131.1	160.4	4.7	5.1	7.0
156-1	2934.6	33.5	-1.9	1.1	2.2
160-1	2558.5	129.3	-14.4	5.1	15.3
160-2	2888.6	276.6	-3.4	9.6	10.2
161-1	2877.7	82.5	-3.8	2.9	4.7
163-1	2836	198.8	-5.2	7.0	8.7
168-1	3027.6	97.4	1.3	3.2	3.5
168-2	3218.1	123.8	7.6	3.8	8.5
171-1	3017.4	98.0	0.9	3.2	3.4
172-1	2208.5	44.4	-26.1	2.0	26.2
174-1	2976.4	64.4	-0.5	2.2	2.2
177-1	2489.7	77.6	-16.7	3.1	17.0

TABLE 2 Analysis of all reported results (continued)

Exposure 2 144 kBq m⁻³ h

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	% biased error	% precision error	% measurement error
7-1	146.9	24.7	2.0	16.8	16.9
13-1	143.7	6.1	-0.2	4.2	4.3
14-1	138.2	9.1	-4.0	6.6	7.7
16-1	143.2	11.9	-0.6	8.3	8.3
16-2	161.9	28.5	12.4	17.6	21.5
16-3	160.6	40.1	11.5	25.0	27.5
19-1	134	11.2	-6.9	8.4	10.9
20-1	132.4	11.3	-8.1	8.5	11.7
23-1	158.6	13.7	10.1	8.6	13.3
25-1	152.2	14.8	5.7	9.7	11.3
25-2	143.5	29.5	-0.3	20.6	20.6
28-1	139.9	25.1	-2.8	17.9	18.2
32-1	140.1	4.9	-2.7	3.5	4.4
40-1	193.2	13.4	34.2	6.9	34.9
45-1	155.9	22.2	8.3	14.2	16.5
122-1	143.1	6.0	-0.6	4.2	4.2
122-2	134.3	6.0	-6.7	4.5	8.1
129-1	134.7	8.6	-6.5	6.4	9.1
141-1	142.9	6.8	-0.8	4.8	4.8
144-1	161.3	19.4	12.0	12.0	17.0
156-1	222.2	38.2	54.3	17.2	57.0
160-1	118.6	48.6	-17.6	41.0	44.6
160-2	207.9	29.1	44.4	14.0	46.5
161-1	160.7	34.3	11.6	21.3	24.3
163-1	29	13.7	-79.9	47.2	92.8
168-1	139.3	9.3	-3.3	6.7	7.4
168-2	131.3	4.0	-8.8	3.0	9.3
171-1	168.7	23.2	17.2	13.8	22.0
172-1	116.4	20.0	-19.2	17.2	25.7
174-1	147	9.4	2.1	6.4	6.7
177-1	128.9	13.8	-10.5	10.7	15.0

TABLE 2 Analysis of all reported results (continued)
Exposure 3 1326 kBq m⁻³ h

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	% biased error	% precision error	% measurement error
7-1	1193.2	39.0	-10.0	3.3	10.5
13-1	1323.2	6.1	-0.2	0.5	0.5
14-1	1265.8	33.6	-4.5	2.7	5.3
16-1	1267.9	32.8	-4.4	2.6	5.1
16-2	1417	58.5	6.9	4.1	8.0
16-3	1351.2	113.1	1.9	8.4	8.6
19-1	1226.4	45.4	-7.5	3.7	8.4
20-1	1170.4	51.6	-11.7	4.4	12.5
23-1	1312.7	42.9	-1.0	3.3	3.4
25-1	1447.5	76.9	9.2	5.3	10.6
25-2	1409.6	122.6	6.3	8.7	10.7
28-1	1416.7	69.7	6.8	4.9	8.4
32-1	1252.7	32.1	-5.5	2.6	6.1
40-1	1769.8	105.1	33.5	5.9	34.0
45-1	1439.7	128.8	8.6	8.9	12.4
122-1	1354.6	30.5	2.2	2.3	3.1
122-2	1246.6	32.0	-6.0	2.6	6.5
129-1	1249.5	38.0	-5.8	3.0	6.5
141-1	1422.4	49.9	7.3	3.5	8.1
144-1	1454.8	69.8	9.7	4.8	10.8
156-1	1559	52.3	17.6	3.4	17.9
160-1	1213.6	71.8	-8.5	5.9	10.3
160-2	1334.4	97.1	0.6	7.3	7.3
161-1	1353.6	69.5	2.1	5.1	5.5
163-1	1420	160.3	7.1	11.3	13.3
168-1	1400.7	55.3	5.6	3.9	6.9
168-2	1437.7	48.2	8.4	3.4	9.1
171-1	1524.4	79.3	15.0	5.2	15.8
172-1	1027.2	36.8	-22.5	3.6	22.8
174-1	1322.1	43.4	-0.3	3.3	3.3
177-1	1146.8	24.3	-13.5	2.1	13.7

TABLE 2 Analysis of all reported results (continued)

Exposure 4 347 kBq m⁻³ h

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	% biased error	% precision error	% measurement error
7-1	322.1	17.4	-7.2	5.4	9.0
13-1	362.6	11.7	4.5	3.2	5.5
14-1	331.8	13.2	-4.4	4.0	5.9
16-1	595.6	707.3	71.6	118.8	138.7
16-2	389.5	24.9	12.2	6.4	13.8
16-3	374.1	36.7	7.8	9.8	12.5
19-1	334.5	10.7	-3.6	3.2	4.8
20-1	318.9	13.3	-8.1	4.2	9.1
23-1	365	20.4	5.2	5.6	7.6
25-1	401.4	35.7	15.7	8.9	18.0
25-2	413.5	117.3	19.2	28.4	34.2
28-1	363.8	38.9	4.8	10.7	11.7
32-1	327.8	10.8	-5.5	3.3	6.4
40-1	449.5	34.8	29.5	7.7	30.5
45-1	376.7	29.4	8.6	7.8	11.6
122-1	356.6	16.8	2.8	4.7	5.5
122-2	337.5	13.1	-2.7	3.9	4.7
129-1	316.7	16.7	-8.7	5.3	10.2
141-1	371.3	13.3	7.0	3.6	7.9
144-1	369.2	36.1	6.4	9.8	11.7
156-1	478.1	65.0	37.8	13.6	40.2
160-1	316.5	21.5	-8.8	6.8	11.1
160-2	389.8	58.5	12.3	15.0	19.4
161-1	372.6	12.9	7.4	3.5	8.1
163-1	279.6	29.8	-19.4	10.7	22.2
168-1	351.3	19.6	1.2	5.6	5.7
168-2	357.4	15.8	3.0	4.4	5.3
171-1	351.7	30.9	1.4	8.8	8.9
172-1	265.4	21.3	-23.5	8.0	24.8
174-1	355.6	11.6	2.5	3.3	4.1
177-1	295.2	20.3	-14.9	6.9	16.4

TABLE 2 Analysis of all reported results (continued)
Exposure 5 657 kBq m⁻³ h

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	% biased error	% precision error	% measurement error
7-1	590.4	20.6	-10.1	3.5	10.7
13-1	636.2	17.0	-3.2	2.7	4.1
14-1	611.1	24.1	-7.0	3.9	8.0
16-1	648.7	21.5	-1.3	3.3	3.5
16-2	663.1	42.2	0.9	6.4	6.4
16-3	695.8	38.6	5.9	5.5	8.1
19-1	604.3	15.0	-8.0	2.5	8.4
20-1	577.1	29.9	-12.2	5.2	13.2
23-1	650.4	29.5	-1.0	4.5	4.6
25-1	753.6	32.3	14.7	4.3	15.3
25-2	653.6	105.8	-0.5	16.2	16.2
28-1	901.2	771.5	37.2	85.6	93.3
32-1	627.9	12.8	-4.4	2.0	4.9
40-1	841.7	42.3	28.1	5.0	28.6
45-1	678.5	74.2	3.3	10.9	11.4
122-1	645.1	21.2	-1.8	3.3	3.8
122-2	602.2	18.4	-8.3	3.1	8.9
129-1	589.6	28.0	-10.3	4.7	11.3
141-1	683.4	27.1	4.0	4.0	5.6
144-1	695.9	41.9	5.9	6.0	8.4
156-1	747.2	90.1	13.7	12.1	18.3
160-1	534.1	35.3	-18.7	6.6	19.8
160-2	605.8	37.0	-7.8	6.1	9.9
161-1	683.2	39.0	4.0	5.7	7.0
163-1	699.4	152.0	6.5	21.7	22.7
168-1	690.4	30.0	5.1	4.3	6.7
168-2	674.9	17.4	2.7	2.6	3.8
171-1	665.2	57.7	1.2	8.7	8.8
172-1	494.2	23.0	-24.8	4.7	25.2
174-1	639	12.1	-2.7	1.9	3.3
177-1	556.8	29.2	-15.3	5.2	16.1

TABLE 2 Analysis of all reported results (continued)

Transit controls

Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)	Set ID	Mean (kBq m ⁻³ h)	1 SD (kBq m ⁻³ h)
7-1	23.4	6.2	122-1	13	1.9
13-1	1.2	2.5	122-2	3.5	1.7
14-1	14.1	4.4	129-1	16.7	15.7
16-1	42.1	22.6	141-1	27.5	11.7
16-2	97.4	21.0	144-1	38	20.0
16-3	42.4	15.7	156-1	29.1	9.6
19-1	21.9	6.4	160-1	71.3	41.5
20-1	3.3	2.0	160-2	34.6	9.9
23-1	31.5	12.4	161-1	21.8	10.9
25-1	9	0.0	163-1	168.7	175.9
25-2	19	0.0	168-1	37.2	6.6
28-1	105.3	22.2	168-2	72.5	26.2
32-1	6	3.2	171-1	16.8	7.4
40-1	5	2.8	172-1	20.9	8.8
45-1	23.5	5.0	174-1	9.6	5.6
			177-1	9.1	7.8

TABLE 3 Statistical analysis of all reported results given in Table 2

Exposure	Mean (μ) of all reported results (kBq m ⁻³ h)	Standard deviation (σ) of all reported results (kBq m ⁻³ h)
1 (2990 kBq m ⁻³ h)	2930	343
2 (144 kBq m ⁻³ h)	146	32
3 (1326 kBq m ⁻³ h)	1346	141
4 (347 kBq m ⁻³ h)	364	62
5 (657 kBq m ⁻³ h)	656	81

TABLE 4 Performance classification scheme based on measurement error

Set ID	Performance classification in each exposure					Detector type	Filter	Holder	Detector material	Detector material supplier
	2	4	5	3	1					
	144 kBq m ⁻³ h	347 kBq m ⁻³ h	657 kBq m ⁻³ h	1326 kBq m ⁻³	2990 kBq m ⁻³ h					
13-1	A	A	A	A	A	Closed		NRPB/SSI	CR-39	Intercast
14-1	A	A	A	A	A	Closed		NRPB/SSI	CR-39	TASL
32-1	A	A	A	A	A	Closed		NRPB/SSI	CR-39	TASL
122-1	A	A	A	A	A	Closed		TASL	CR-39	TASL
122-2	A	A	A	A	A	Closed		TASL	CR-39	TASL
168-1	A	A	A	A	A	Closed		TASL	CR-39	TASL
168-2	A	A	A	A	A	Closed		Eperm S	Electret	N/A
174-1	A	A	A	A	A	Closed		TASL	CR-39	TASL
141-1	A	A	A	A	B	Closed		TASL	CR-39	TASL
129-1	A	B	B	A	A	Closed		Own	CR-39	Intercast
16-1	A	F	A	A	D	Closed	Yes	Radosys	CR-39	Radosys
23-1	B	A	A	A	A	Closed		NRPB/SSI	CR-39	TASL
19-1	B	A	A	A	B	Closed		Own	CR-39	Intercast
7-1	B	A	B	B	B	Closed		TASL	CR-39	TASL
20-1	B	A	B	B	B	Closed		TASL	CR-39	TASL
144-1	B	B	A	B	A	Closed	Yes	Radosys	CR-39	Radosys

Set ID	Performance classification in each exposure					Detector type	Filter	Holder	Detector material	Detector material supplier
	2	4	5	3	1					
	144 kBq m ⁻³ h	347 kBq m ⁻³ h	657 kBq m ⁻³ h	1326 kBq m ⁻³	2990 kBq m ⁻³ h					
45-1	B	B	B	B	A	Closed		Own	LR 115	LR115
25-1	B	B	B	B	B	Open		Dosirad	LR115	Dosirad
177-1	B	B	B	B	B	Closed		TASL	CR-39	TASL
28-1	B	B	F	A	C	Closed	Yes	Radosys	CR-39	Radosys
161-1	C	A	A	A	A	Closed	Yes	Radosys	CR-39	Radosys
171-1	C	A	A	B	A	Closed		Own	LR115	Dosirad
16-2	C	B	A	A	A	Closed	Yes	Radosys	CR-39	Radosys
16-3	C	B	A	A	A	Closed	Yes	Radosys	CR-39	Radosys
172-1	C	C	C	C	C	Closed	Yes	Radosys	CR-39	Radosys
25-2	C	D	B	B	B	Closed		Dosirad	LR115	Dosirad
40-1	D	D	C	D	D	Closed		NRPB/SSI	CR-39	Mi-Net
160-2	E	B	A	A	B	Closed		NRPB/SSI	CR-39	TASL
160-1	E	B	B	B	B	Closed		TASL	CR-39	TASL
163-1	F	C	C	B	A	Closed		Eperm S	Electret	N/A
156-1	F	E	B	B	A	Closed		KfK FN	Makrofol	KIT

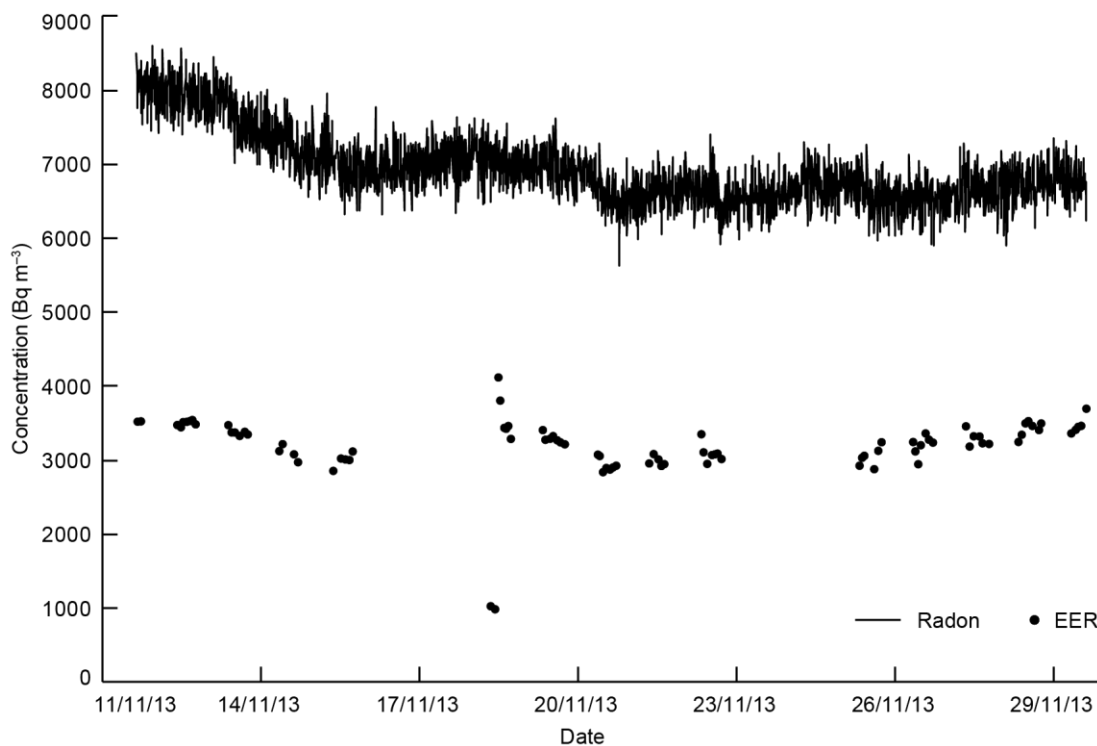


FIGURE 1 Radon and EER concentrations for exposure 1

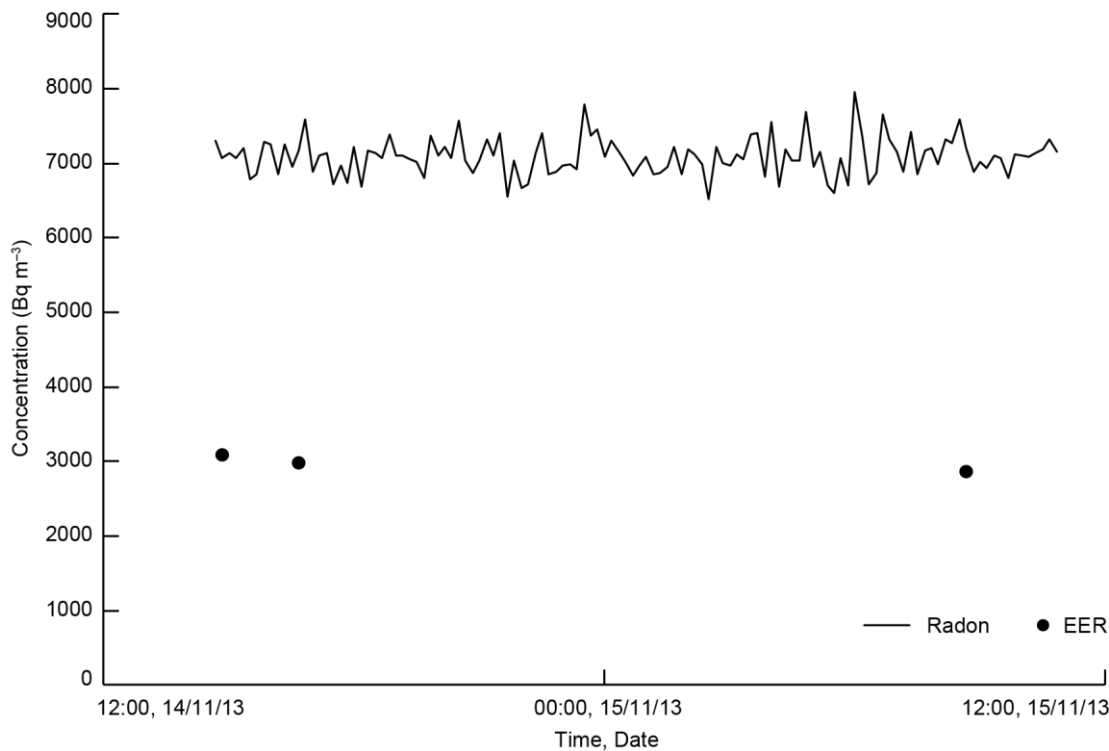


FIGURE 2 Radon and EER concentrations for exposure 2

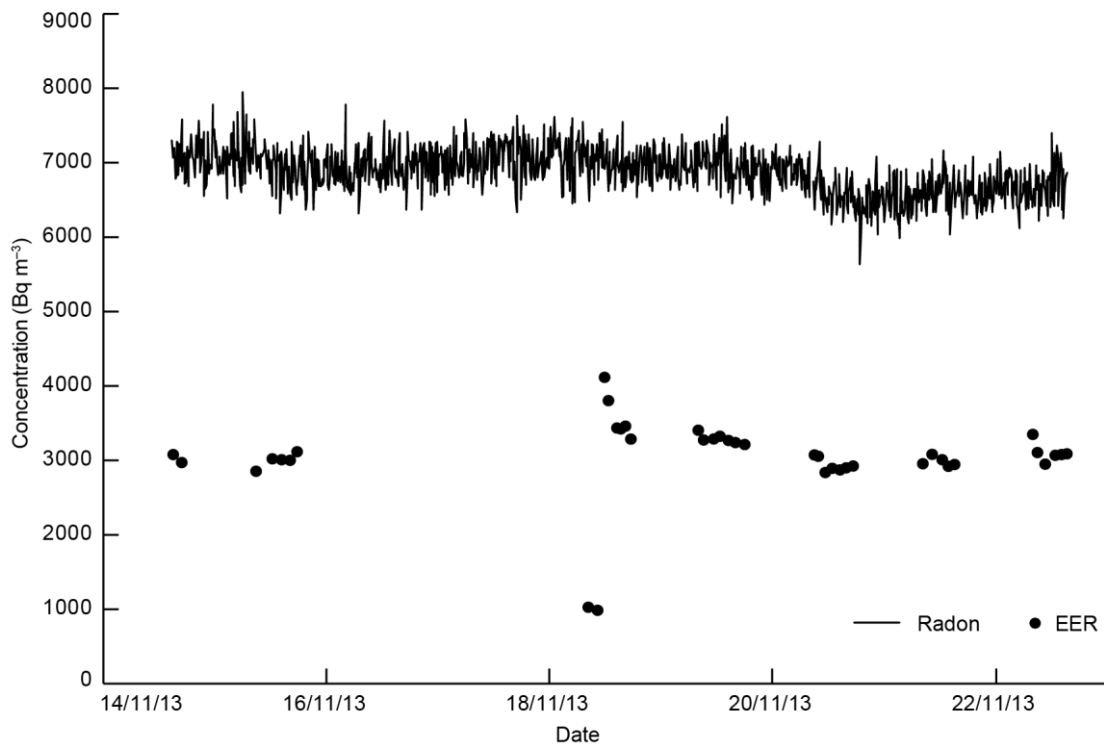


FIGURE 3 Radon and EER concentrations for exposure 3

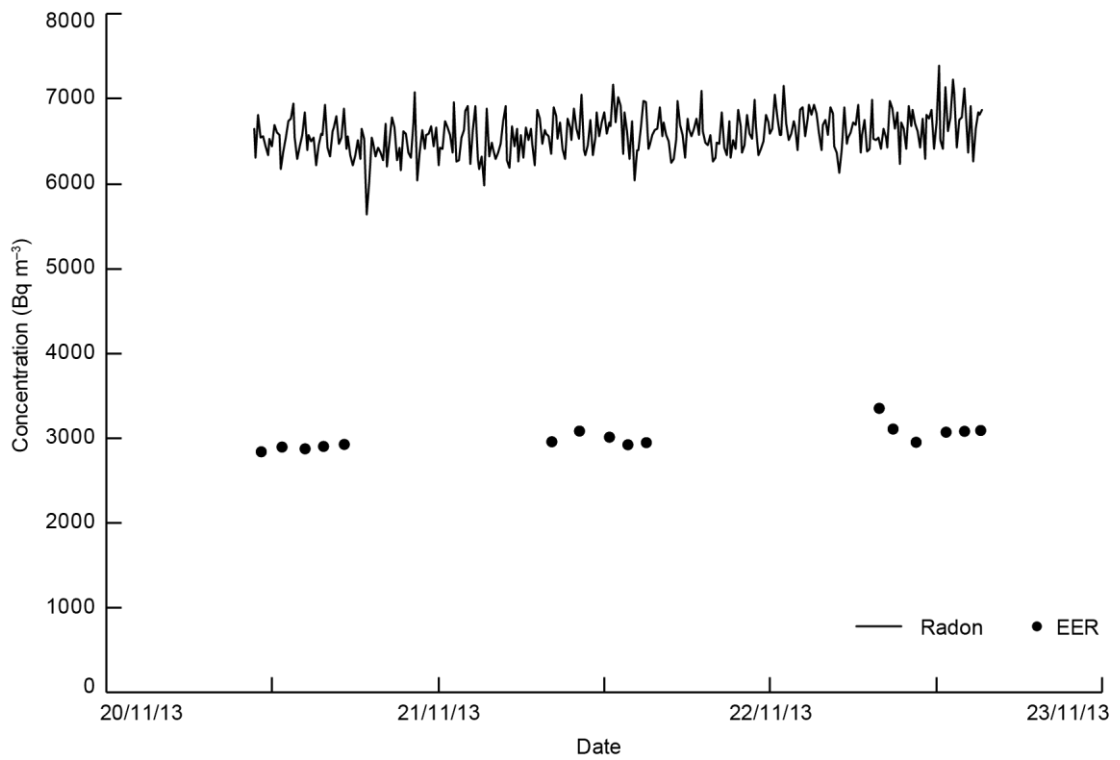


FIGURE 4 Radon and EER concentrations for exposure 4

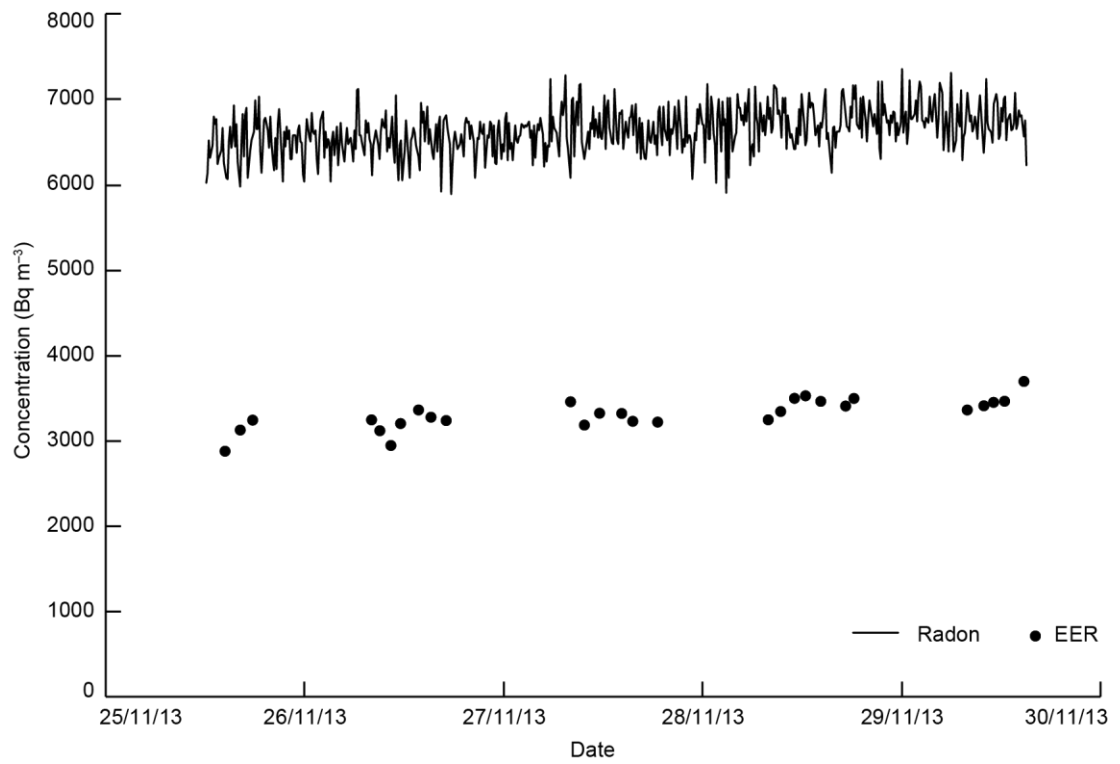


FIGURE 5 Radon and EER concentrations for exposure 5

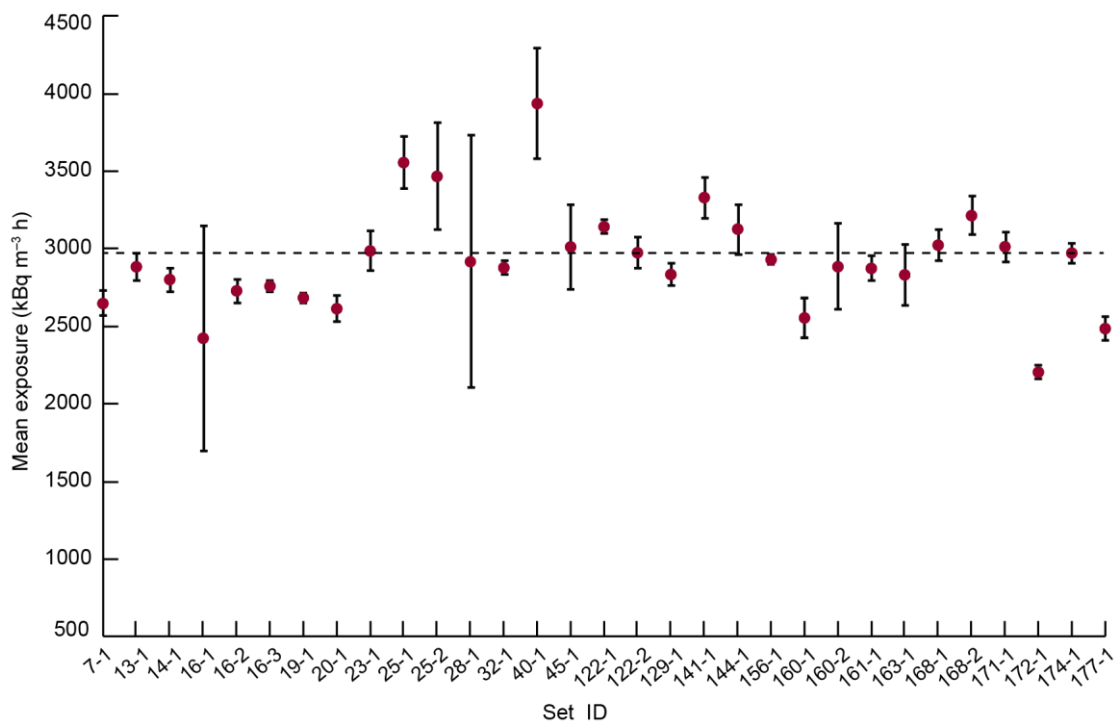


FIGURE 6 Results as reported by participants for exposure 1

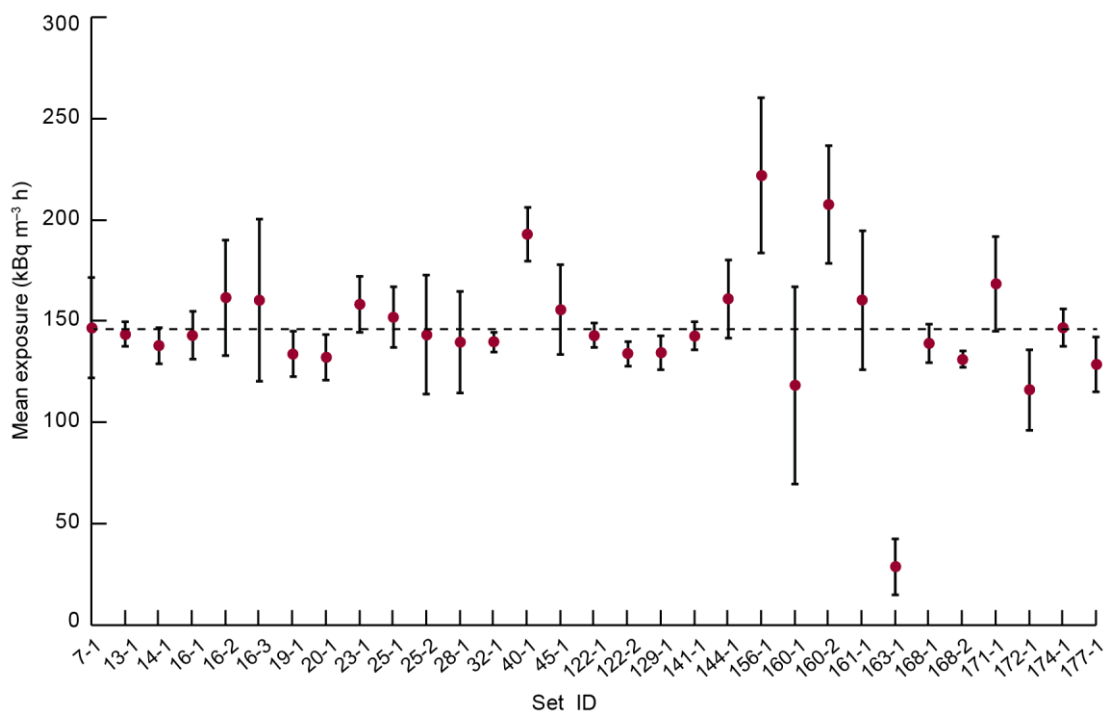


FIGURE 7 Results as reported by participants for exposure 2

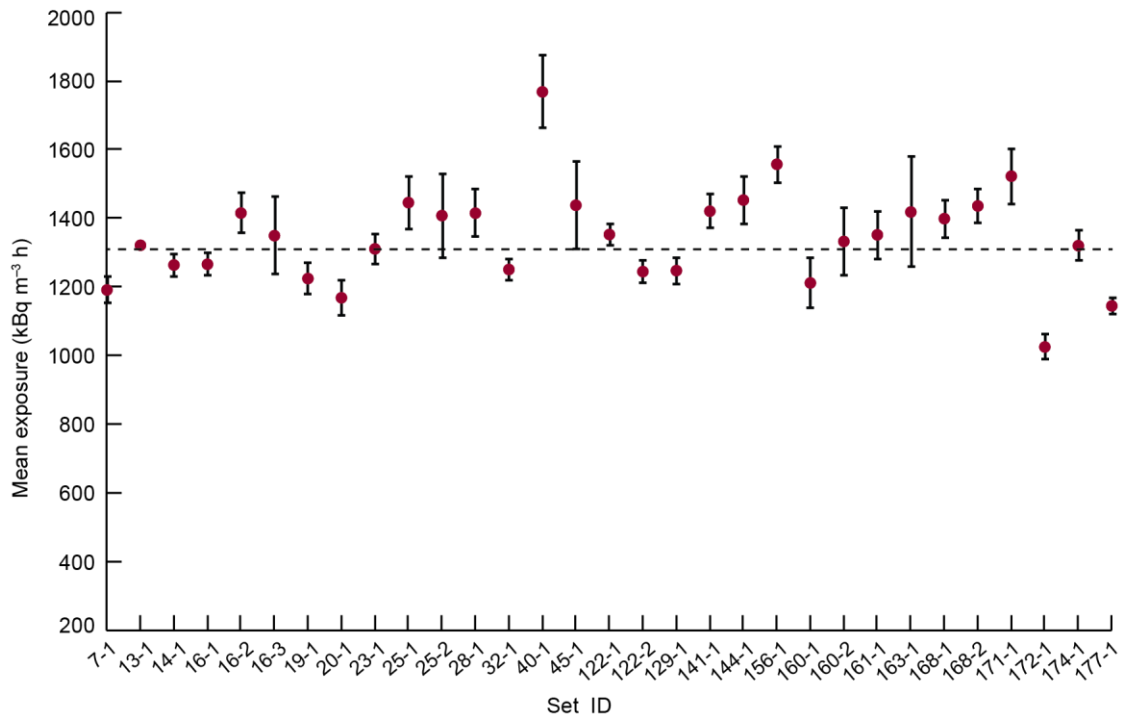


FIGURE 8 Results as reported by participants for exposure 3

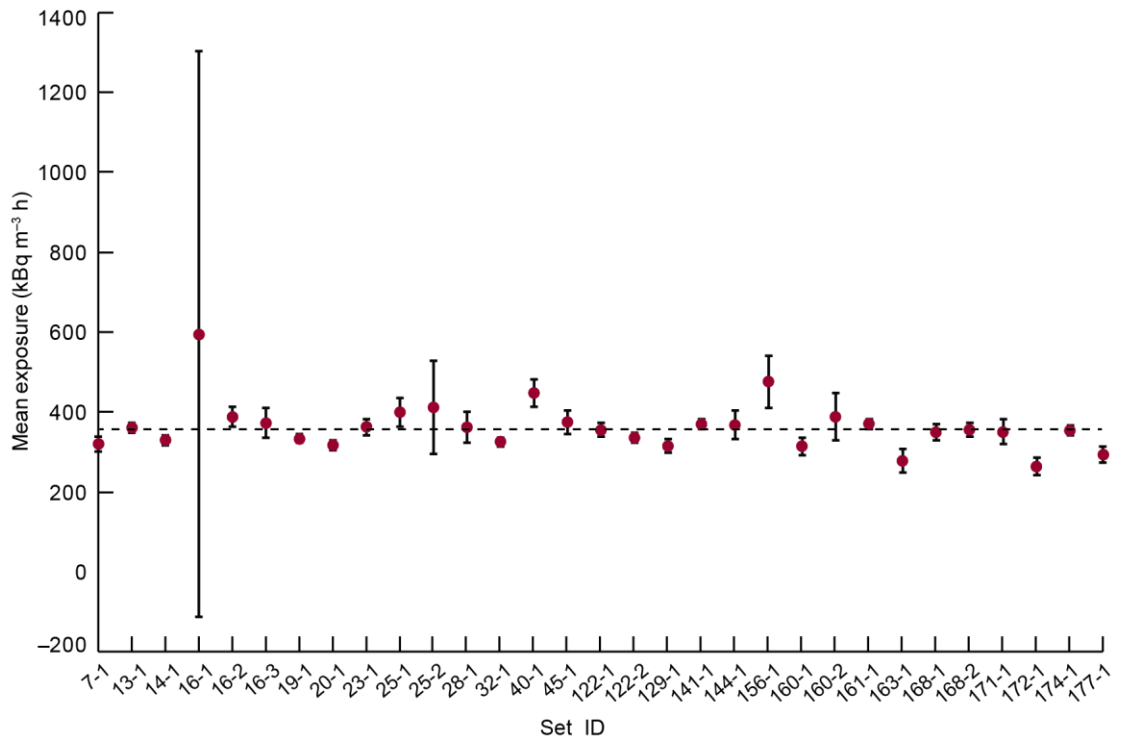


FIGURE 9 Results as reported by participants for exposure 4

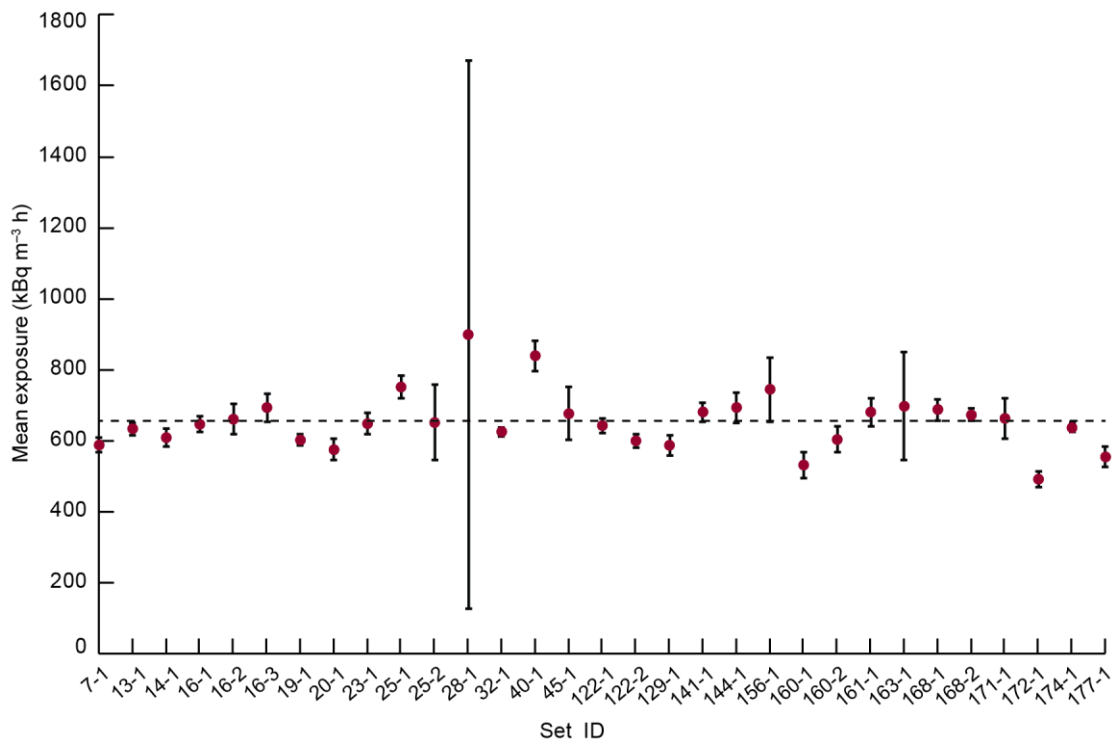


FIGURE 10 Results as reported by participants for exposure 5

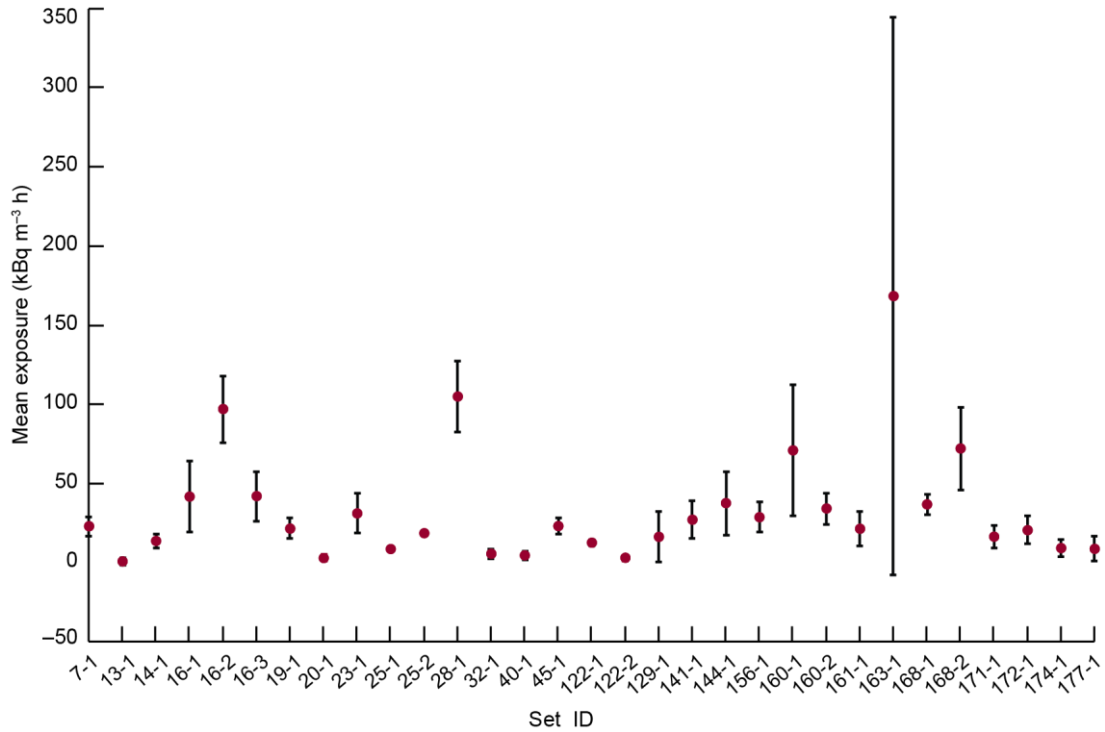


FIGURE 11 Results as reported by participants for transit exposure

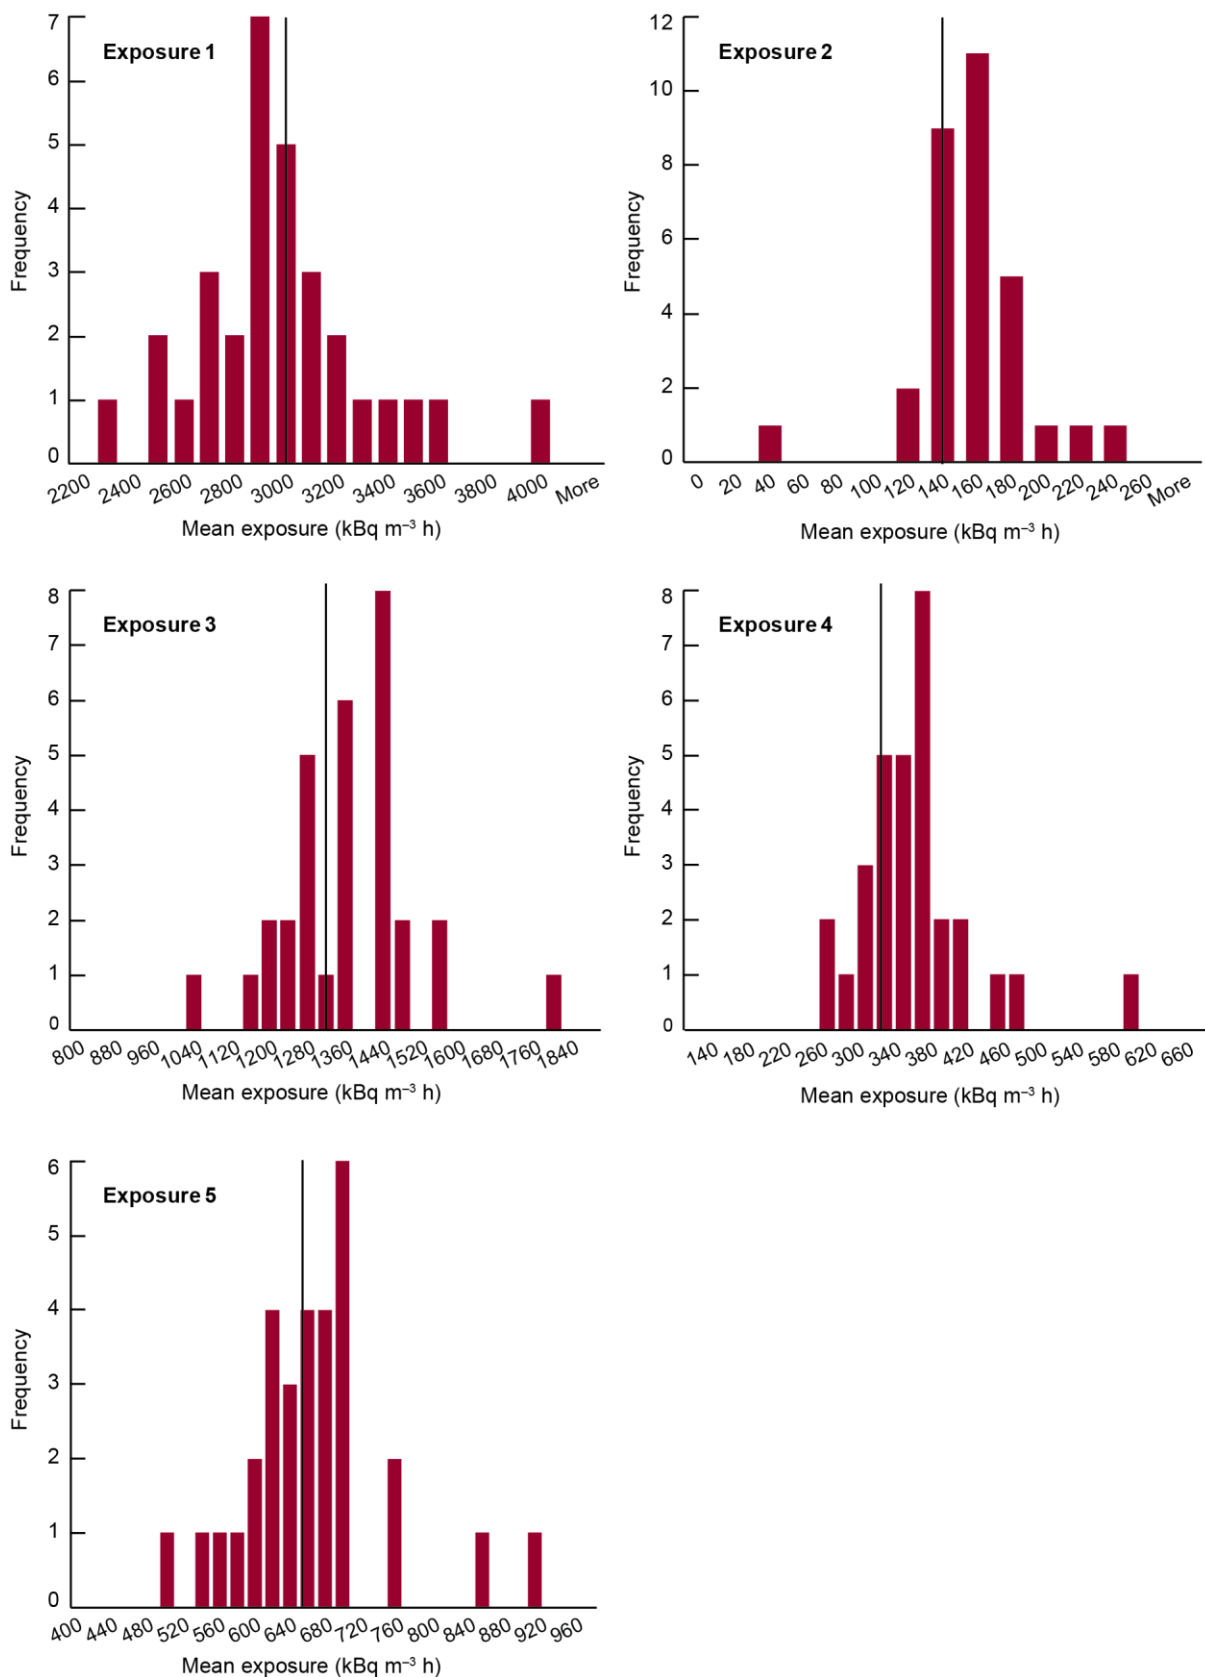


FIGURE 12 Distribution of mean exposure results given in Table 3

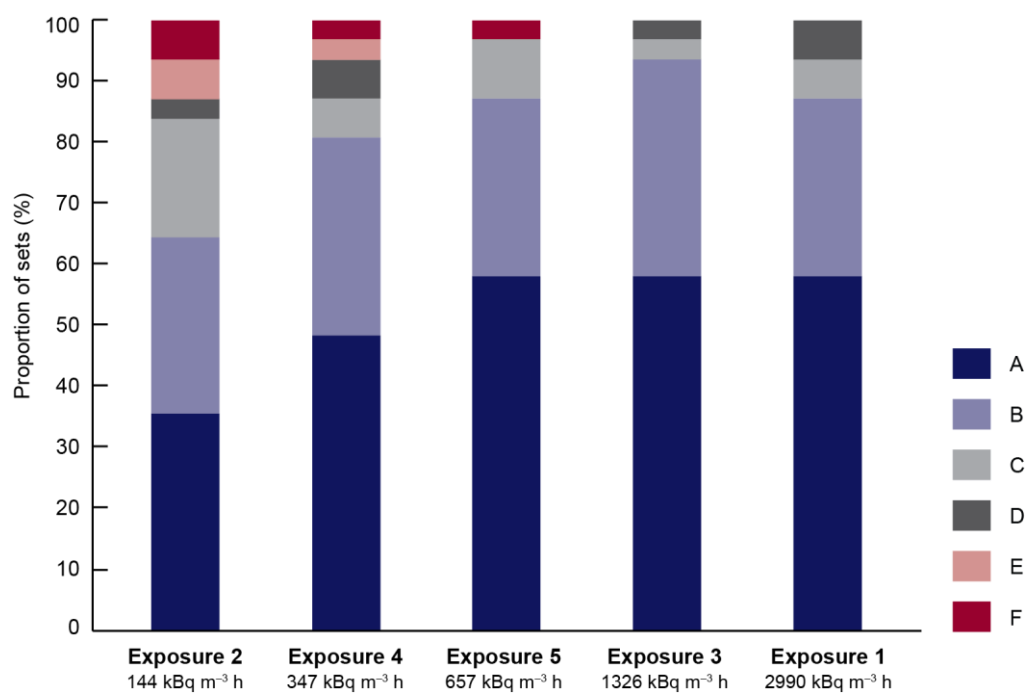


FIGURE 13 Proportions of sets achieving different performance classes for each exposure