



EU Type Examination Certificate Number: **0120/SGS0430**

Gacia Electrical Appliance Co., LTD.

No.1 Nanxijiang Road
Daqiao Industrial Zone
Yueqing, Wenzhou
China

Instrument Identification:
N8DM-34 Series

Polyphase, Active Import / Export (kWh), Indoor, Electricity Meter

Instrument Traceable Number
0120/SGS0430

has been assessed and certified as meeting the requirements of

EU Directive 2014/32/EU **on Measuring Instruments Annex II, Module B**

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of Annex V of EU Directive 2014/32/EU

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex II, Module D or Annex II, Module F


This certificate is valid until 5th January 2025
Issue 1

Certification is based on report number(s) SHES130800321501 dated 26th December 2014
EMA198278/1 dated 26th December 2014
EMA198278/2 dated 21st June 2016
EMA275962

Authorised Signature


SGS United Kingdom Limited, Notified Body 0120
Unit 202B Worle Parkway, Weston-super-Mare, BS22 6WA, UK
t +44 (0)1934 522917 f +44 (0)1934 522137 www.sgs.com

Contact Address
SGS United Kingdom Limited, Units 12A & 12B, South Industrial Estate, Bowburn, Durham, DH6 5AD, UK
t +44 (0)191 377 2000 f +44 (0)191 377 2020 www.sgs.com


	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020


1. Technical Data

Manufacturer	Gacia Electrical Appliance Co., LTD
Meter Type	N8DM-34Standard, N8DM-34MT, N8DM-34Modbus, N8DM-34Mbus, N8DM-34Pulse, N8DM-34-2T
Voltage Rating (U_n)	3x230/400V
Current Rating (I_{min} – I_{ref} (I_{max}))	0.5-10(100)A & 0.5-10(80)A
Frequency (F_n)	50Hz
Active Accuracy Class (kWh)	A or B (kWh)
Type of circuit	3p4w, 3p3w, 1p2w
Temperature Range	-25°C to +55°C
Software/ Firmware Version No CRC Checksum Identification Location	N8DM-34Standard, N8DM-34MT, N8DM-34Modbus, N8DM-34Mbus, N8DM-34Pulse: V1.3 N8DM-34-2T: V1.4 N8DM-34Standard, N8DM-34MT, N8DM-34Modbus, N8DM-34Pulse: 0x0000AFF9 N8DM-34Mbus: 0x00003C02 N8DM-34-2T: 0x00009DF4 Nameplate
Bill Of Materials Number	N8DM-34Standard, N8DM-34MT, N8DM-34Modbus, N8DM-34Mbus, N8DM-34Pulse: V1.4 N8DM-34-2T: DH-JS-180008-1.0
IP Rating	IP51
Insulation Protective Class	Class II
LED Pulse Constant	400imp/ kWh
Impulse Voltage Rating	6kV
AC Voltage Rating	4kV
Main Cover Sealing Type	1 x Wire & Crimp
Integrity of meter	Inaccessible without breaking seals
Intended Location of the Meter	Indoor
Type of Register	LCD
Terminal Arrangement(s)	DIN
Location of Manufacturers Address	On accompanying documentation

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020

2. Photograph of Meter and Sealing Plan

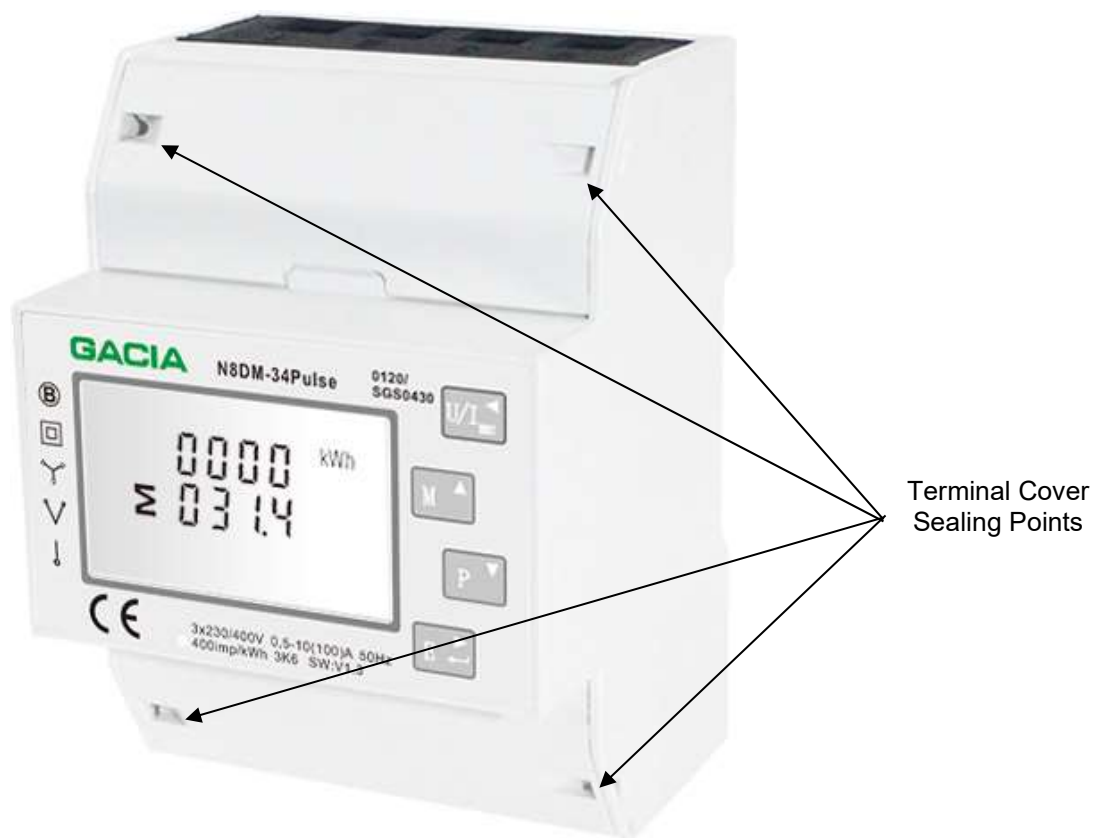

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020

3. Examples of Nameplates




GACIA
N8DM-34Pulse 0120/SGS0430
Three Phase Energy Meter
 3x230/400V AC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.3 CAT III
 CE M20 0120 B □ Y △ 3K6
Gacia Electrical Appliance Co., LTD
No.1 Nanxijiang Road, Wenzhou, Zhejiang



GACIA
N8DM-34Standard 0120/SGS0430
Three Phase Energy Meter
 3x230/400V AC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.3 CAT III
 CE M20 0120 B □ Y △ 3K6
Gacia Electrical Appliance Co., LTD
No.1 Nanxijiang Road, Wenzhou, Zhejiang



GACIA
N8DM-34Modbus 0120/SGS0430
Three Phase Energy Meter
 3x230/400V AC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.3 CAT III
 CE M20 0120 B □ Y △ 3K6
Gacia Electrical Appliance Co., LTD
No.1 Nanxijiang Road, Wenzhou, Zhejiang

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020




GACIA
N8DM-34Mbus 0120/SGS0430
Three Phase Energy Meter
 3x230/400VAC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.3 CAT III
 CE M20 0120 B □ Y △ 3K6
 Gacia Electrical Appliance Co., LTD
 No.1 Nanxijiang Road, Wenzhou, Zhejiang



GACIA
N8DM-34MT 0120/SGS0430
Three Phase Energy Meter
 3x230/400VAC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.3 CAT III
 CE M20 0120 B □ Y △ 3K6
 Gacia Electrical Appliance Co., LTD
 No.1 Nanxijiang Road, Wenzhou, Zhejiang



GACIA
N8DM-34-2T 0120/SGS0430
Three Phase Energy Meter
 3x230/400VAC 0,5-10(100)AAC 50Hz 2020
 400imp/kWh EN50470-1/3 IP51 SW:1.4 CAT III
 CE M20 0120 B □ Y △ 3K6
 Gacia Electrical Appliance Co., LTD
 No.1 Nanxijiang Road, Wenzhou, Zhejiang

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020


4. Calculation of the composite error/ MPE

During the type approval examination the influence factors for temperature, frequency and voltage are determined per load point. The table below represents the sum of the square values per load, determined via the following formula:-


$$\delta e(T, U, f) = \sqrt{(\delta e^2(T, I, \cos\phi) + \delta e^2(U, I, \cos\phi) + \delta e^2(f, I, \cos\phi))}$$

where

$\delta e(T, I, \cos\phi)$	=	Additional error due to variation of the temperature at the same load
$\delta e(U, I, \cos\phi)$	=	Additional error due to variation of the voltage at the same load
$\delta e(f, I, \cos\phi)$	=	Additional error due to variation of the frequency at the same load

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020

		Influence Factors for Temperature. Frequency & Voltage					
Current	PF Cos	-25°C	-10°C	5°C	30°C	40°C	55°C
I _{min}	1.0	0.46	0.34	0.14	0.18	0.29	0.52
I _{tr}	1.0	0.57	0.39	0.19	0.11	0.24	0.46
10I _{tr}	1.0	0.64	0.45	0.25	0.06	0.20	0.42
I _{max}	1.0	0.75	0.60	0.44	0.26	0.23	0.30
I _{tr}	0.5ind	0.56	0.40	0.20	0.14	0.24	0.49
10I _{tr}	0.5ind	0.60	0.43	0.23	0.11	0.23	0.45
I _{max}	0.5ind	0.62	0.47	0.30	0.05	0.10	0.28
I _{tr}	0.8cap	0.65	0.46	0.27	0.11	0.21	0.43
10I _{tr}	0.8cap	0.62	0.44	0.24	0.12	0.24	0.46
I _{max}	0.8cap	0.69	0.55	0.37	0.16	0.14	0.28
L1							
I _{tr}	1.0	0.84	0.60	0.32	0.08	0.20	0.48
10I _{tr}	1.0	0.97	0.71	0.46	0.10	0.13	0.36
I _{max}	1.0	0.93	0.70	0.48	0.16	0.06	0.25
I _{tr}	0.5ind	0.60	0.32	0.09	0.25	0.42	0.66
10I _{tr}	0.5ind	0.79	0.56	0.29	0.12	0.27	0.53
I _{max}	0.5ind	0.84	0.63	0.40	0.10	0.11	0.33
L2							
I _{tr}	1.0	0.40	0.26	0.09	0.08	0.16	0.37
10I _{tr}	1.0	0.42	0.31	0.19	0.08	0.17	0.36
I _{max}	1.0	0.44	0.36	0.25	0.08	0.08	0.23
I _{tr}	0.5ind	0.20	0.09	0.24	0.27	0.35	0.53
10I _{tr}	0.5ind	0.43	0.30	0.17	0.10	0.20	0.40
I _{max}	0.5ind	0.46	0.35	0.25	0.09	0.06	0.20
L3							
I _{tr}	1.0	0.55	0.37	0.15	0.14	0.30	0.51
10I _{tr}	1.0	0.51	0.33	0.11	0.20	0.33	0.56
I _{max}	1.0	0.55	0.39	0.21	0.10	0.21	0.52
I _{tr}	0.5ind	0.41	0.24	0.06	0.32	0.46	0.66
10I _{tr}	0.5ind	0.41	0.22	0.04	0.31	0.46	0.67
I _{max}	0.5ind	0.43	0.30	0.34	0.17	0.30	0.53


	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020

5. Annex of Variants

Product Variant Identification Details:

Type Designation	Description of meter
N8DM-34MT:	Three phase, multi-function, multi-tariff, 2 pulse outputs and 1 RS485 Modbus communication port
N8DM-34Modbus:	Three phase, multi-function, 2 pulse outputs and 1 RS485 communication port
N8DM-34Mbus:	Three phase, multi-function, 2 pulse outputs and 1 Mbus communication port
N8DM-34Pulse:	Three phase, multi-function, 2 pulse outputs
N8DM-34Standard:	Three phase, 2 pulse outputs and 1 RS485 communication port
N8DM-34-2T:	Three phase, multi-function, dual tariffs, 2 pulse outputs and 1 RS485 communication port

Modifications to the meter(s) described according to approval No.**0120/SGS0430** must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

	EU-Type Examination Certificate Number:	
	0120/SGS0430	
	Issue Number: 1	Dated: 9 th April 2020

6. Document Revision History

Issue	Date	Comments
1	09/04/2020	Initial Issue

This document is issued by the Company subject to its General Conditions for Certification Services, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.

Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested *and such sample(s) are retained for 28 days only*.

END OF CERTIFICATE